
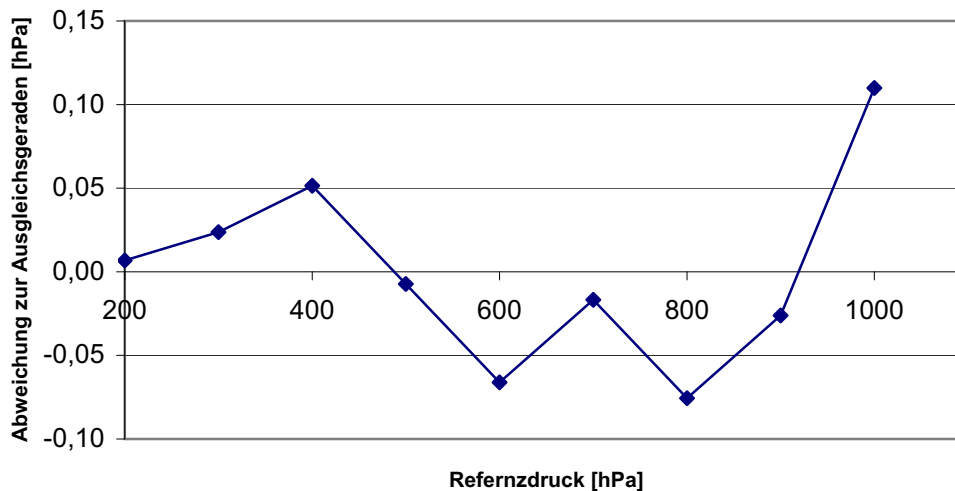


Kalibrierprotokoll		
Sensor Rosemount 1201F2A1B1A	Serien-Nr. 956	
Druckreferenz MPS 30	Serien-Nr. 5029	Messbereich 0-1084 hPa
Spannungsmessgerät Keithley 2000	Serien-Nr. 703709	T <sub>Umgeb.</sub> [°C] 21
Dateiname Keithley_20090106_5.adf	Kanal 2	

Referenz [hPa]	Spannung [V]	Berechnet [hPa]	Abweichung [hPa]
1000	4,6204	1000,1	0,11
900	4,158	900,0	-0,03
800	3,696	799,9	-0,08
700	3,2345	700,0	-0,02
600	2,7725	599,9	-0,07
500	2,311	500,0	-0,01
400	1,8495	400,1	0,05
300	1,3876	300,0	0,02
200	0,92575	200,0	0,01

Werte der Ausgleichsgeraden

Offset      -0,47110584      hPa  
Steigung    216,5572356      hPa/V



06.01.2009

Datum

Name