
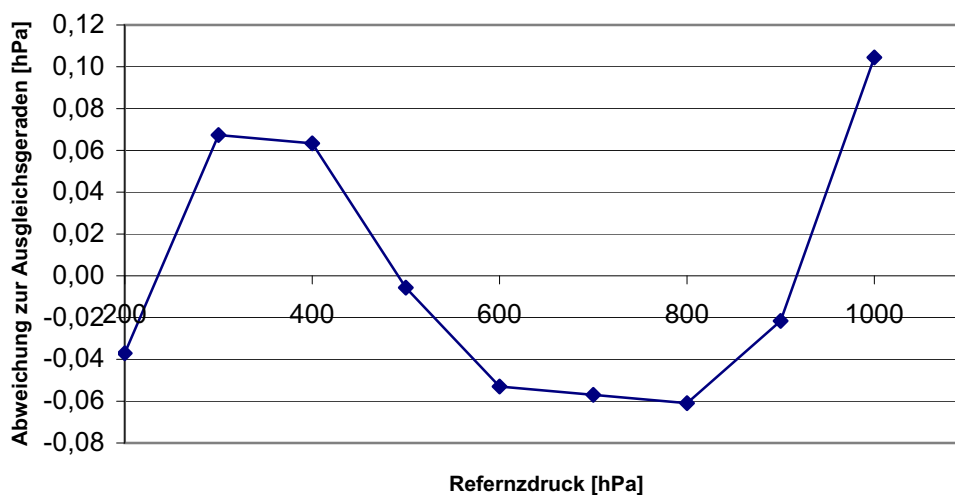


Kalibrierprotokoll		
Sensor Rosemount 1201F2A1B1A	Serien-Nr. 1019	
Druckreferenz MPS 30	Serien-Nr. 5029	Messbereich 0-1084 hPa
Spannungsmessgerät Keithley 2000	Serien-Nr. 703709	T _{Umgeb.} [°C] 21
Dateiname Keithley_20090106_5.adf	Kanal 1	

Referenz [hPa]	Spannung [V]	Berechnet [hPa]	Abweichung [hPa]
1000	4,6048	1000,1	0,10
900	4,1427	900,0	-0,02
800	3,681	799,9	-0,06
700	3,2195	699,9	-0,06
600	2,758	599,9	-0,05
500	2,2967	500,0	-0,01
400	1,8355	400,1	0,06
300	1,374	300,1	0,07
200	0,912	200,0	-0,04

Werte der Ausgleichsgeraden

Offset	2,354337338	hPa
Steigung	216,6761049	hPa/V



06.01.2009

Datum

Name