
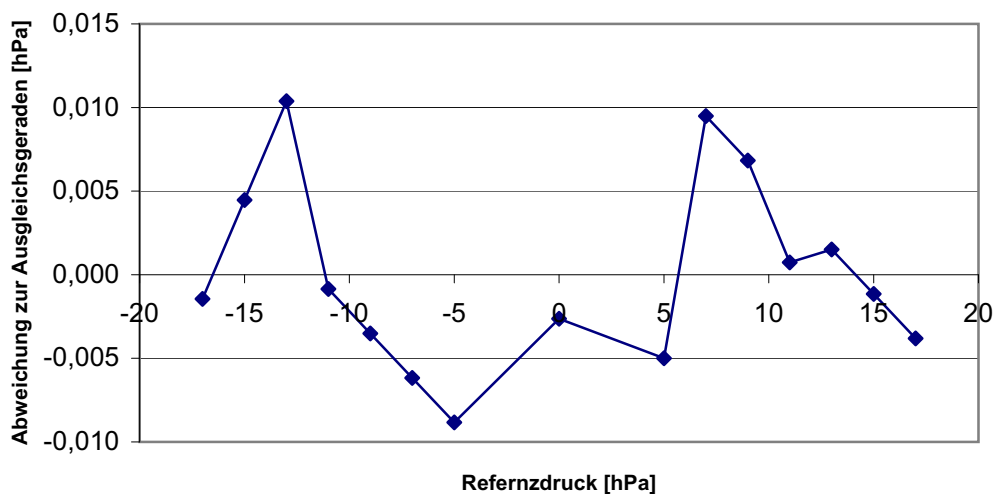


Kalibrierprotokoll		
Sensor Rosemount 1221F2VL3B1B	Serien-Nr. 495 / Beta	
Druckreferenz MPS 30	Serien-Nr. 5029	Messbereich +/-17,2 hPa
Spannungsmessgerät Keithley 2000	Serien-Nr. 703709	T _{Umgeb.} [°C] 21
Dateiname Keithley_20090106_diff.adf	Kanal 2	

Referenz [hPa]	Spannung [V]	Berechnet [hPa]	Abweichung [hPa]
17	9,91	17,0	-0,004
15	8,745	15,0	-0,001
13	7,58	13,0	0,002
11	6,413	11,0	0,001
9	5,250	9,0	0,007
7	4,085	7,0	0,009
5	2,91	5,0	-0,005
0	-0,005	0,0	-0,003
-5	-2,925	-5,0	-0,009
-7	-4,09	-7,0	-0,006
-9	-5,255	-9,0	-0,004
-11	-6,42	-11,0	-0,001
-13	-7,58	-13,0	0,010
-15	-8,75	-15,0	0,004
-17	-9,92	-17,0	-0,001

Werte der Ausgleichsgeraden

Offset 0,005943442 hPa
Steigung 1,714454386 hPa/V



06.01.2009

Datum

Name