
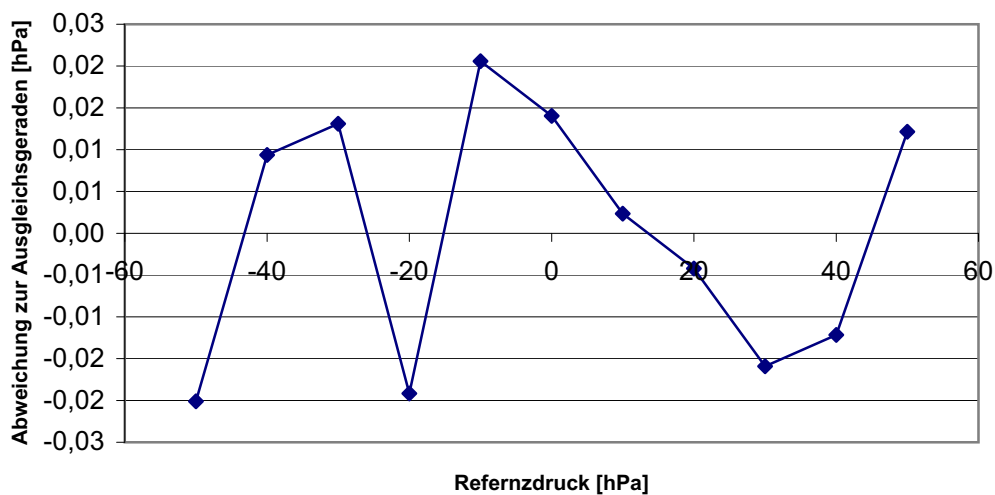


Kalibrierprotokoll		
Sensor Rosemount 1221VL6B1B	Serien-Nr. 666	
Druckreferenz MPS 30	Serien-Nr. 5029	Messbereich +/-51,7 hPa
Spannungsmessgerät Keithley 2000	Serien-Nr. 703709	T _{Umgeb.} [°C] 21
Dateiname Keithley_20090106_4.adf	Kanal 0	

Referenz [hPa]	Spannung [V]	Berechnet [hPa]	Abweichung [hPa]
50	9,724	50,0	0,01
40	7,775	40,0	-0,01
30	5,83	30,0	-0,02
20	3,888	20,0	0,00
10	1,945	10,0	0,00
0	0,003	0,0	0,01
-10	-1,94	-10,0	0,02
-20	-3,892	-20,0	-0,02
-30	-5,83	-30,0	0,01
-40	-7,775	-40,0	0,01
-50	-9,725	-50,0	-0,02

Werte der Ausgleichsgeraden

Offset	-0,00140272	hPa
Steigung	5,143310318	hPa/V



06.01.2009

Datum

Name